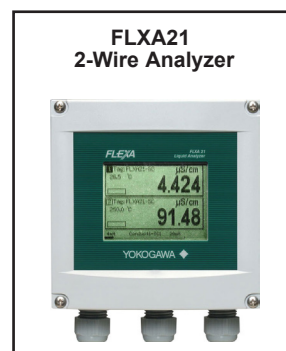
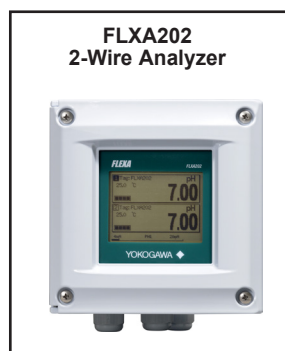
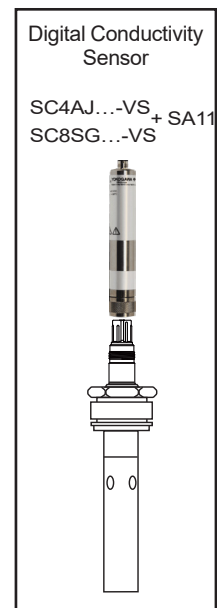


Technical Information

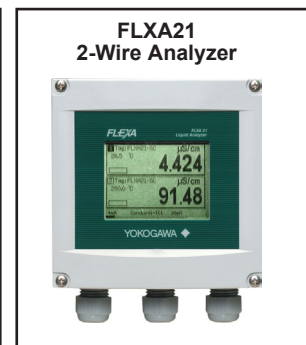
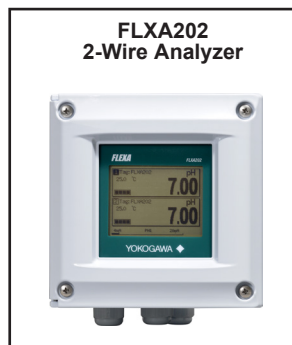
Conductivity Analyzer Selection Guide

TI 12D08A01-02E

■ Conductivity / Resistivity Analyzers



■ Inductive Conductivity Analyzers



*1: Model ISC40SJ is available only in Japan.

FLEXA, FLXA, SENCOM are trademarks or registered trademarks of Yokogawa Electric Corporation.

All other company and product names mentioned in this document are trademarks or registered trademarks of their respective companies.

■ Conductivity Sensor Selection Guide and Compatible Instruments

	2-Electrode System					
Model Name	SC4AJ-□-□□-□□-002	SC4AJ-□-□□-□□-010	SC10XB	SC8SG-R31-T	SC8SG-R61-T	
	SC4AJ-□-□□-□□-002-□□- -VS+SA11*5	SC4AJ-□-□□-□□-010-□□- -VS+SA11*5		SC8SG-R31-T- □□□-VS+SA11*5		

Specifications

Cell constant	0.02 cm ⁻¹	0.1 cm ⁻¹	0.05 cm ⁻¹	0.01 cm ⁻¹	10 cm ⁻¹	
Minimum measuring range	0 to 0.5 μS/cm	0 to 5 μS/cm	0 to 2.0 μS/cm	0 to 0.5 μS/cm	0 to 1 mS/cm	
Maximum measuring range	0 to 200 μS/cm	0 to 1000 μS/cm	0 to 2000 μS/cm	0 to 100 μS/cm	0 to 1000 mS/cm	
Process temperature	0 to 110 °C	0 to 110 °C	0 to 70 °C	0 to 100 °C	0 to 100 °C	
Process pressure	0 to 1 MPa	0 to 1 MPa	0 to 500 kPa	0 to 1 MPa*1	0 to 1 MPa*1	
Cable length	3/5/10/15/20 m No extension cable available		3/5/10 m Extension cable*2	5.5/10/20 m No extension cable available		
Installation	Adapter mounting type Welding socked type Clamp type		Drop- in type Piping connection with optional adapter	Screw-in type Flow-through type (screw) Flow-through type (flange)		

Applications

High purity water (0.1-50 μS/cm)	A	B	N	A	N	
Tap water, industrial water	B	A	B	N	B	
Industrial effluent, sewage	N	N	N	N	B	
Acid/alkaline solution, brackish water, seawater	N	N	N	N	N	
Food processing plant (interface detection)*3	N	N	N	N	N	
Food processing plant (control of cleaning chemicals)	N	N	N	N	N	

Converter Compatibility

FLXA402 4-Wire Converter (conductivity/resistivity)	B	B	N	B	B	
FLXA202 2-Wire Analyzer (conductivity/resistivity)	B *5	B *5	N	B *5	B	
FLXA21 2-Wire Analyzer (conductivity/resistivity)	B *5	B *5	N	B *5	B	

Rating: A=Recommended, B=Applicable, X=Not applicable

*1: In case of PP (polypropylene) chamber, process pressure range is 0 to 500 kPa.

*2: Total length including extension cable should not exceed 50 m.

*3: Use SC500 Sanitary Conductivity Converter. SC500 is available only in Japan.

*4: Please refer to General Specification GS 12D06B01-01E or GS 12D08J02-E-E for the process temperature limit when these sensors are used in Hazardous Area.

*5: SA11 (SENCOM Smart Adapter) cannot be used for FLXA202/FLXA21 or does not apply to inductive conductivity.

Note • The table above is for reference purposes only. Consult YOKOGAWA for more selection information.

• See the following references for further selection information:

FLXA402 : GS 12A01F01-01EN, FLXA202: GS 12A01A03-01EN, FLXA21 : GS 12A01A02-01E

SC sensors : GS 12D08G02-E, ISC sensors : GS 12D06B01-01E

2-Electrode System		4-Electrode System	Inductive Conductivity System					
	SC210G-A	SC210G-B	SC8SG-R61-F	ISC40GJ	ISC40SJ	ISC40G	ISC40S	Model Name
			SC8SG-R61-F-□□□-VS+SA11*5					
Specifications								
	0.05 cm ⁻¹	5 cm ⁻¹	10 cm ⁻¹					Cell constant
	0 to 0.5 μS/cm	0 to 200 μS/cm	0 to 1 mS/cm	0 to 100 μS/cm	0 to 100 μS/cm	0 to 100 μS/cm	0 to 100 μS/cm	Minimum measuring range
	0 to 200 μS/cm	0 to 20 mS/cm	0 to 1000 mS/cm	0 to 1999 mS/cm	0 to 1999 mS/cm	0 to 1999 mS/cm	0 to 1999 mS/cm	Maximum measuring range
	0 to 100 °C	0 to 100 °C	0 to 100 °C	-10 to 130 °C	-10 to 130 °C*4	-20 to 130 °C (PEEK) -20 to 100 °C (PFA)	-20 to 130 °C (PEEK)*4 -20 to 100 °C (PFA)*4	Process temperature
	0 to 1 MPa*1	0 to 1 MPa*1	0 to 1 MPa*1	0 to 2 MPa	0 to 2 MPa	0 to 2 MPa (PEEK) 0 to 1 MPa (PFA)	0 to 2 MPa (PEEK) 0 to 1 MPa (PFA)	Process pressure
	3/5/10/15/20 m No extension cable available		5.5/10/20 m No extension cable available	5/10/15/20 m Extension cable*2	5/10/15/20 m No extension cable available	5/10/15/20 m Extension cable available	5/10/15/20 m Extension cable available	Cable length
	Screw in type Flange type Flow-through type (screw or flange) Screw in type with gate valve		Screw-in type Flow-through type (screw) Flow-through type (flange)	with optional screw-in adapter with optional flange adapter with optional dedicated submersion type holder				Installation
Applications								
	B	N	N	N	N	N	N	High purity water (0.1-50 μS/cm)
	B	A	B	B	B	B	B	Tap water, industrial water
	N	B	A	A	A	A	A	Industrial effluent, sewage
	N	N	N	A	A	A	A	Acid/alkaline solution, brackish water, seawater
	N	N	N	N	N	N	N	Food processing plant (interface detection)*3
	N	N	N	A	A	A	A	Food processing plant (control of cleaning chemicals)
Converter Compatibility								
	B	B	B	B	N	B	B *6 *8	FLXA402 4-Wire Converter (conductivity/resistivity)
	B	B	B *5	B	B	B	B *7 *8	FLXA202 2-Wire Analyzer (conductivity/resistivity)
	B	B	B *5	B	N	B	B *7 *8	FLXA21 2-Wire Analyzer (conductivity/resistivity)

Rating: A=Recommended, B=Applicable, X=Not applicable

*6: NI for FM only

*7: IS for FM, CSA, ATEX, IECEx

*8: The cable length should not exceed 50 m.











■ Conductivity Converter Selection Guide

	Model Name	FLXA402	FLXA202	FLXA21
	Product Name	4-Wire converter	2-wire analyzer	2-wire analyzer
Installation site	Indoors	R	A	A
	Outdoors (non-hazardous area)	R	R	R
	Outdoors (hazardous area)	A*	R	R
Application	For integration	A	/	/
	Small-scale instrumentation			
	General purpose Medium-scale instrumentation	R	A	A

Rating: R=Recommended, A=Applicable, N=Not applicable
 *: NI for FM only

■ Four-wire Conductivity / Resistivity Analyzers

● System Configuration

Conductivity Sensors						Conductivity Converter
<div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p>SC4AJ*</p>  <p>Adapter Mounting Type</p>  <p>Welding Socket Type</p>  <p>Welding Clamp Type</p> </div> <div style="width: 45%;"> <p>SC8SG*</p>  <p>Screw-in Type</p>  <p>Flow-through Type</p> </div> </div>					<p>FLXA402 4-Wire Converter</p> 	
<div style="display: flex; justify-content: space-around;"> <div style="width: 20%;"> <p>SC210G</p>  <p>Screw-in Type</p> </div> <div style="width: 20%;">  <p>Flange Type</p> </div> <div style="width: 20%;">  <p>Flow-through Type</p> </div> <div style="width: 20%;">  <p>Screw-in Type with Gate Valve</p> </div> </div>						

*: Applicable to SA11.

Two-wire Conductivity / Resistivity Analyzers

System Configuration – Non-explosion protected type








Conductivity Sensors						Conductivity Converter	Distributor
<p>SC4AJ</p> <p>Adapter Mounting Type Welding Socket Type Welding Clamp Type</p>				<p>SC8SG</p> <p>Screw-in Type Flow-through Type</p>		<p>FLXA202 / FLXA21</p>	<p>Dedicated Distributor PH201G</p> <p>Analog output 1 to 5 V DC Output Failure contact output Maintenance contact output</p>
<p>SC210G</p> <p>Screw-in Type Flange Type Flow-through Type Screw-in Type with Gate Valve</p>				<p>General Distributor SDBT, SDBS</p> <p>Analog output 1 to 5 V DC Output</p>			

System Configuration – Explosion protected type

Conductivity Sensors				Conductivity Converter	Distributor Safety Barrier
<p>SC4AJ</p> <p>Adapter Mounting Type Welding Socket Type Welding Clamp Type</p>				<p>FLXA202 / FLXA21</p>	<p>Refer to TI 12A01A02-42EN FLXA202 Selection Guide for Intrinsic Safety-type Associated Apparatus.</p> <p>For FLXA21, use TI 12A01A02-42EN as a reference.</p>
<p>SC210G</p> <p>Screw-in Type Flange Type Flow-through Type Screw-in Type with Gate Valve</p>					










■ Four-wire Inductive Conductivity Analyzer

● System Configuration





Inductive Conductivity Sensor	Holders	Inductive Conductivity Converter
 <p>ISC40GJ</p>	<p>Immersion ISC40FDJ</p>  <p>Flow-Through ISC40FFJ</p>  <p>Direct Insertion ISC40FSJ</p>  <div style="border: 1px solid black; padding: 5px; margin: 10px auto; width: fit-content;"> <p>Terminal Box</p> <p>Terminal Box BA20</p>  </div> <p>Extension Cable WF10J</p> 	<p>FLXA402 4-Wire Converter</p> 

■ Two-wire Inductive Conductivity Analyzers

● System Configuration – Non-explosion protected type

Inductive Conductivity Sensor	Holders	Inductive Conductivity Converter	Distributor
 <p>ISC40GJ</p>	<p>Immersion ISC40FDJ</p>  <p>Flow-Through ISC40FFJ</p>  <p>Direct Insertion ISC40FSJ</p>  <div style="border: 1px solid black; padding: 5px; margin: 10px 0;"> <p>Terminal Box</p> <p>Terminal Box BA20</p>  </div> <p>Extension Cable WF10J</p> 	<p>FLXA202 / FLXA21</p> 	<p>Dedicated Distributor PH201G</p>  <p>Analog output 1 to 5 V DC Output Failure contact output Maintenance contact output</p> <p>General Distributor SDBT, SDBS</p>  <p>Analog output 1 to 5 V DC Output</p>

● System Configuration – Explosion protected type

Inductive Conductivity Sensor	Holders	Inductive Conductivity Converter	Distributor Safety Barrier
<p>ISC40S</p> 	<p>Flow-Through ISC40FFJ</p>  <p>Direct Insertion ISC40FSJ</p> 	<p>FLXA202 / FLXA21</p> 	<p>Refer to TI 12A01A02-42EN FLXA202 Selection Guide for Intrinsic Safety-type Associated Apparatus.</p> <p>For FLXA21, use TI 12A01A02-42EN as a reference.</p>

Revision Information

- Title : Conductivity Analyzer Selection Guide
- Manual No. : TI 12D08A01-02E

Feb. 2020/6th Edition

FLXA402, SA11 were added.

SC450G, ISC450G were deleted.

Aug. 2018/5th Edition

Corrected errors, etc. (page 2, 5, 7)

Jan. 2018/4th Edition

Corrected an error by deleting ISC40FDJ. (table of page 7 System Configuration - Explosion proof)

Dec. 2017/3rd Edition

FLXA202 is added. SC202G, SC202S, SC202SJ are deleted. "Transmitter" was replaced with "Analyzer."

Oct. 2011/2nd Edition

SC100 is deleted (termination of product).

Dec. 2008/1st Edition

Newly published

■ Yokogawa Electric Corporation
2-9-32 Nakacho, Musashino-shi, Tokyo 180-8750, JAPAN
<http://www.yokogawa.com/>
