
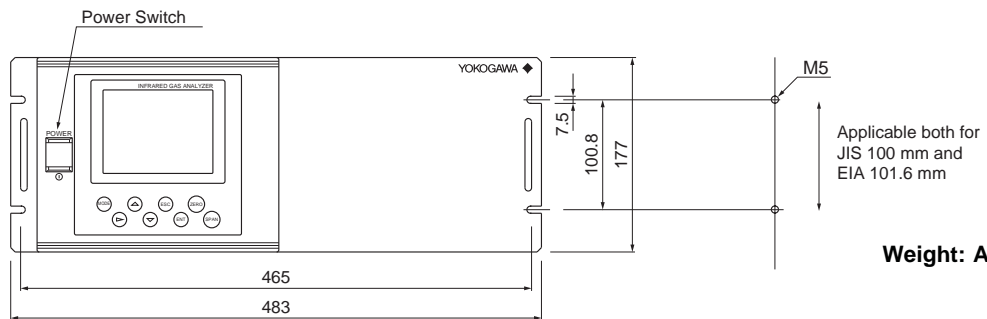



Drawings

Model IR200 Infrared Gas Analyzer

Unit : mm

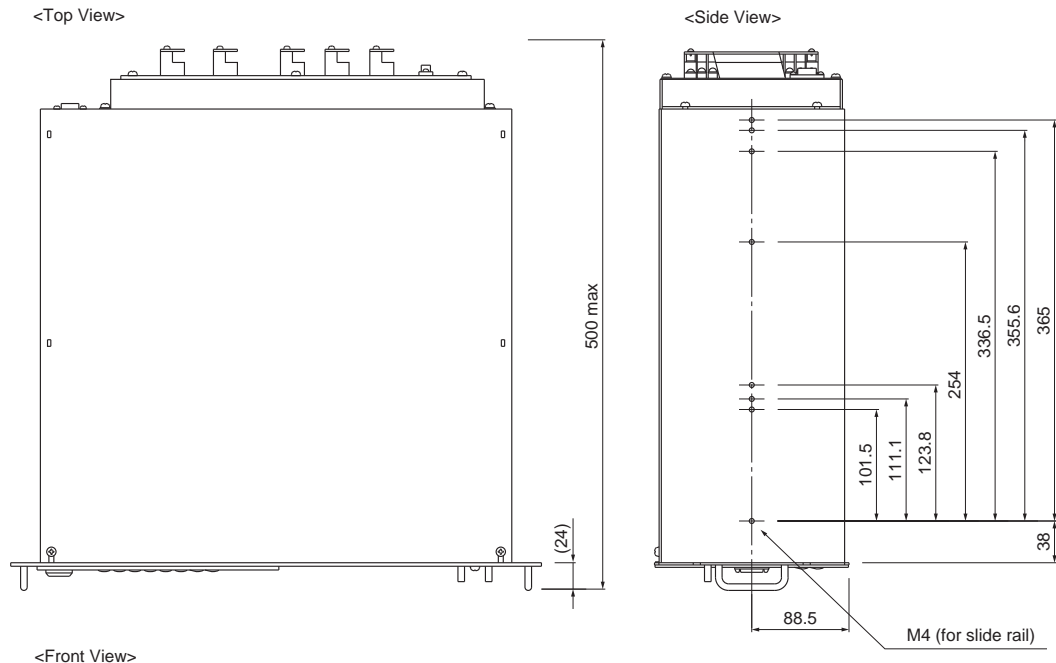

Weight: Approx. 10 kg

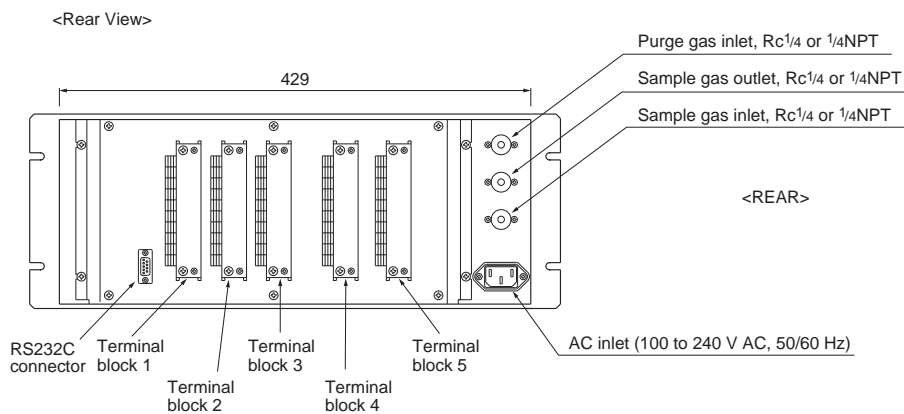


F04.EPS

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = \pm (Criteria of tolerance class IT18 in JIS B0401) / 2.


ACCESSORY SLIDE RAIL

Model : 305A-20/Accuride International Inc.

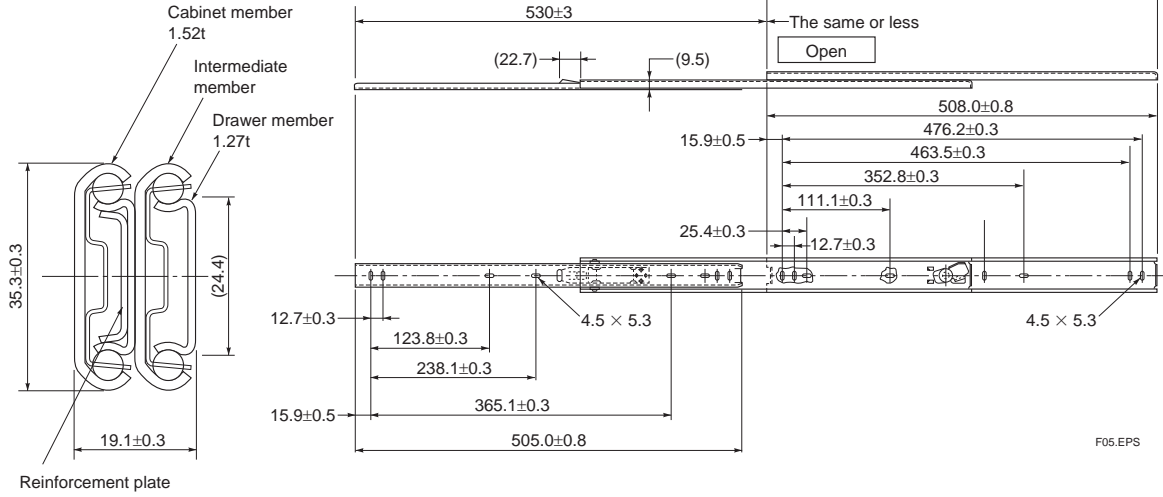


19-inch rack mounting method: The mass of the instrument should be supported at the bottom of the unit (or the side of the unit when mounted with the slide rails).

Also, for facilitate maintenance, a structure which allows extraction of the main unit by using the slide rail is recommended.

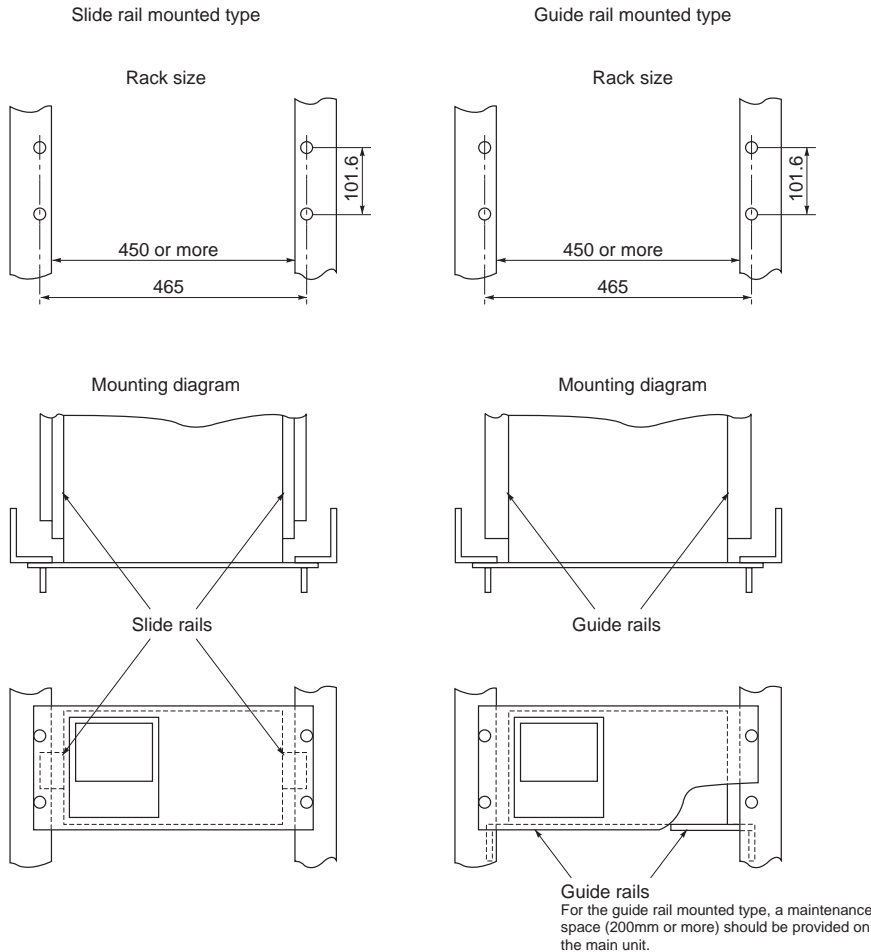

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = ± (Criteria of tolerance class IT18 in JIS B0401) / 2.

EXTERNAL CONNECTION DIAGRAM

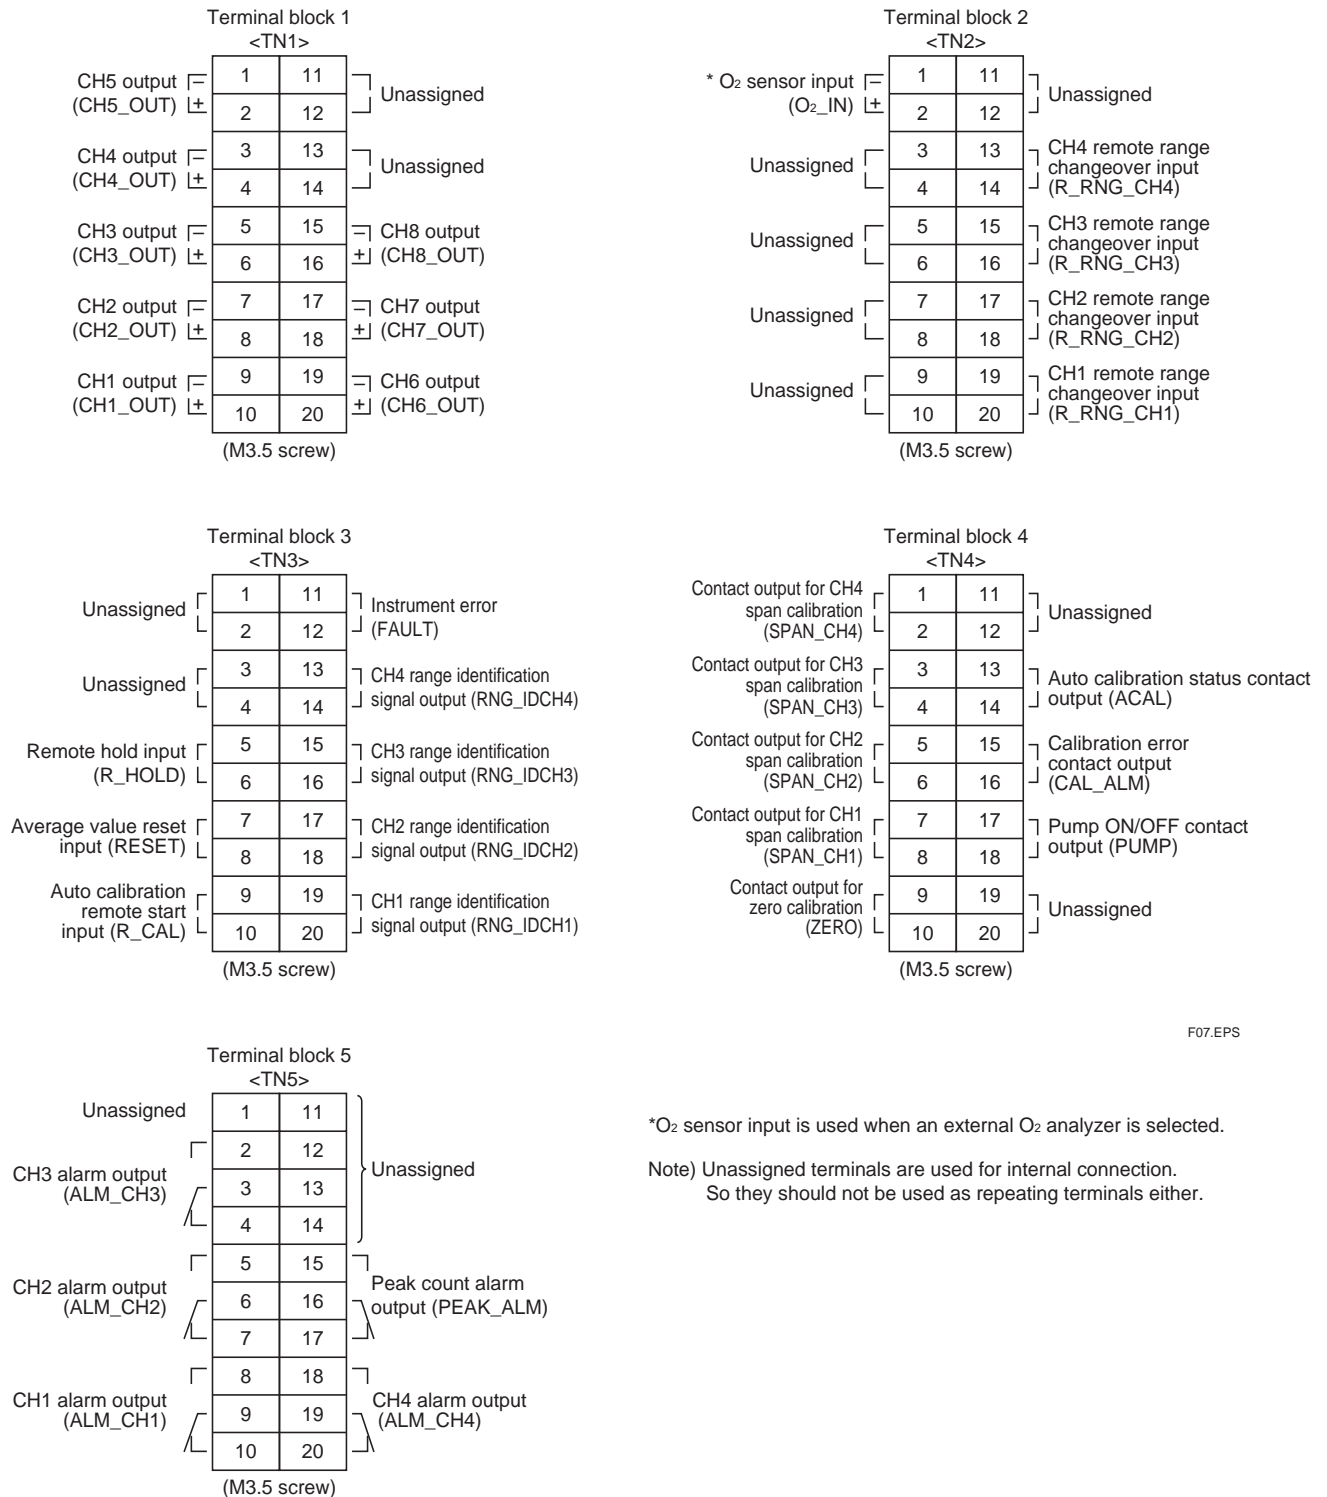

Unless otherwise specified, differences in the dimensions are specified as: General tolerance = ± (Criteria of tolerance class IT18 in JIS B0401) / 2.